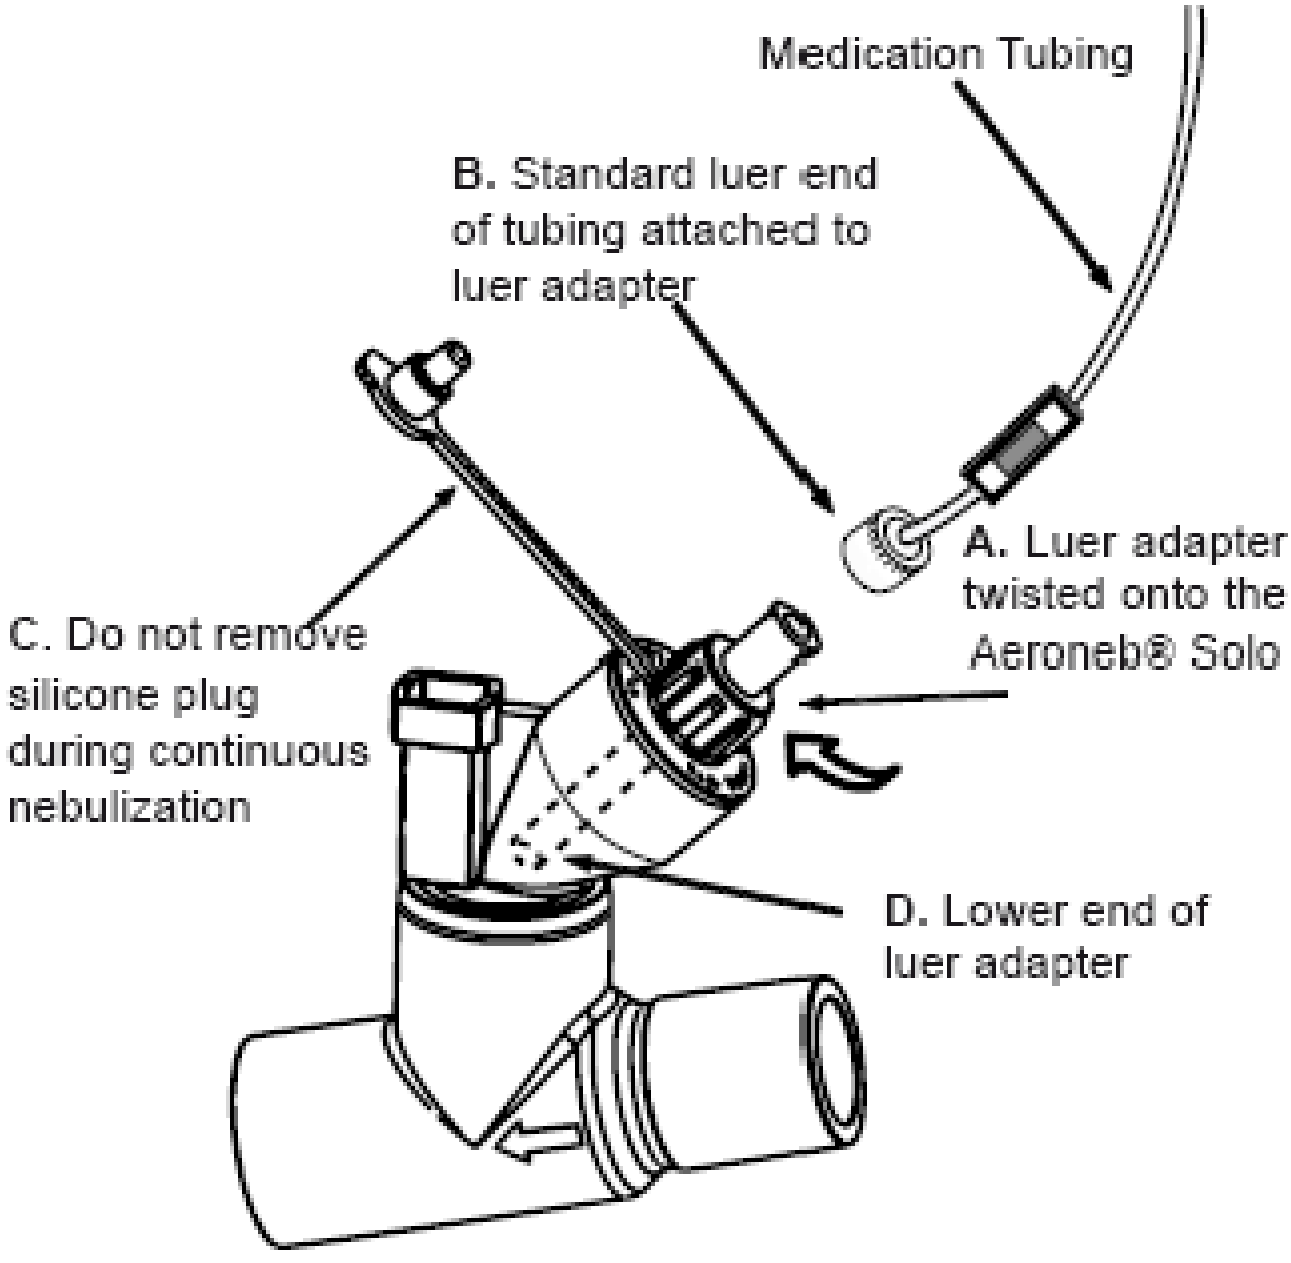
Medication Tubing
B. Standard luer end of tubing attached to luer adapter
A. Luer adapter twisted onto the Aeroneb® Solo
C. Do not remove silicone plug during continuous nebulization
D. Lower end of luer adapter